
## Introducers



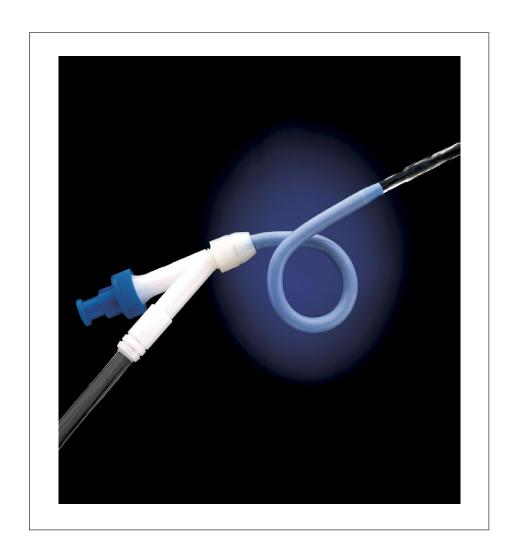

# Contents

Соок Access Plus <sup>©</sup> – Luer Lock High-Volume Infusion Introducer with Hemostasis Valve Set and Tray
Cook Access Plus® – Luer Lock High-Volume Infusion Introducer Tray
Intro Deuce® – Luer Lock Double Lumen Introducer with Hemostasis Valve Tray
Check-Flo® Performer® Accessory Adapter
Sterility Sleeve
Peel-Away® Introducer Sets 9
References
Videotapes

#### **COOK ACCESS PLUS®**

#### LUER LOCK HIGH-VOLUME INFUSION INTRODUCER WITH HEMOSTASIS VALVE SET AND TRAY




Used to introduce balloon, electrode, closed or non-tapered end and other catheters.

- Cook Access Plus® Introducers feature a uniquely fabricated sheath designed to provide maximum flexibility without kinking or compression.
- Gradual tapering of dilator reduces transition from wire guide to sheath for ease of insertion.
- The sheath accepts catheters with diameters of 7.0-9.0 French.
- Recommended for pulmonary artery balloon catheters larger than 7.0 French.
- The hemostasis valve prevents blood reflux and air aspiration and minimizes compression of thermodilution catheters.
- Luer lock fitting on valve assembly prevents dilator slippage during insertion while providing secure fixation of sterility sleeve.
- Large bore side-arm design is ideally suited for unimpeded fluid infusion

The maximum diameter of the instrument or catheter to be introduced should be determined to insure its passage through the sheath.1

Supplied sterile in peel-open packages. Intended for one-time use.

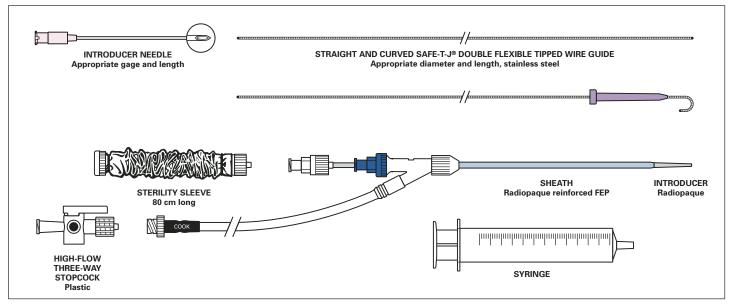


ORDER NUMBER	<sup>1</sup> INTRODUCER French Size	WIRE Diameter	GUIDE Tip	SHEATH Length	Remarks	Global Product Number
Set						
C-FYBLI-9.0-35-J-10.5	9.0	.035 inch	straight and 3 mm "J"	10.5 cm	Introducer with Coons taper	G09321
Tray²						
C-FYBLIY-9.0-35-J-10.5	9.0	.035 inch	straight and 3 mm "J"	10.5 cm	Introducer with Coons taper	G09313

<sup>&</sup>lt;sup>2</sup>Tray consists of items shown above and the following items: 25 gage needle, 22 gage needle, lidocaine, povidone-iodine swabsticks, fenestrated drape, gauze sponges, disposable syringe, suture with needle, povidone-iodine ointment, CSR wrap and prep tray.

Patent Numbers 4,705,511; 4,657,772

#### **COOK ACCESS PLUS®**

#### **LUER LOCK HIGH-VOLUME INFUSION INTRODUCER TRAY**




Used for high-volume replacement of fluids and introduction of balloon, electrode, closed or non-tapered end and other catheters.

- Cook Access Plus® Introducers feature a uniquely fabricated sheath designed to provide maximum flexibility without kinking or compression.
- Luer lock fitting on the dilator prevents slippage during introduction over the wire guide.

The maximum diameter of the instrument or catheter to be introduced should be determined to insure its passage through the sheath.<sup>1</sup>

Supplied sterile in peel-open packages. Intended for one-time use.

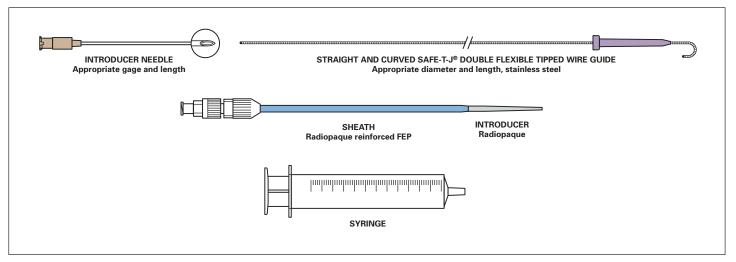


ORDER NUMBER	<sup>1</sup> INTRODUCER French Size	WIRE GUIDE Diameter Tip		SHEATH Length	DILATOR Type	Global Product Number
Tray <sup>2</sup>						
C-FSSIY-9.0-35-J-13.0	9.0	.035 inch	straight and 3 mm "J"	13.0 cm	Coons	G09467

<sup>&</sup>lt;sup>2</sup>Tray consists of items shown above and the following items: 25 gage needle, 22 gage needle, lidocaine, povidone-iodine swabsticks, fenestrated drape, gauze sponges, disposable syringe, suture with needle, povidone-iodine ointment, CSR wrap and prep tray.

Patent Numbers 4,705,511; 4,657,772

#### **INTRO DEUCE®**

#### **LUER LOCK DOUBLE LUMEN INTRODUCER WITH HEMOSTASIS VALVE TRAY**




Used to introduce balloon, electrode, closed or non-tapered end and other catheters.

- The sheath incorporates two separate, noncommunicating vascular access lumens within a single catheter body.
- The large lumen of the sheath accepts catheters with diameters of 7.0-8.5 French.
- Small lumen of the sheath allows venous pressure monitoring, blood sampling and infusion of drugs and fluids.
- Small lumen equivalent size is 18 gage.
- Exit port of small lumen is spaced one centimeter from end of sheath.
- The hemostasis valve prevents blood reflux and air aspiration and minimizes compression of thermodilution catheters.
- Luer lock fitting on valve assembly prevents dilator slippage during insertion while providing secure fixation of sterility sleeve.
- Large bore side-arm design is ideally suited for unimpeded fluid infusion.

The maximum diameter of the instrument or catheter to be introduced should be determined to insure its passage through the sheath.<sup>1</sup>

Supplied sterile in peel-open packages. Intended for one-time use.

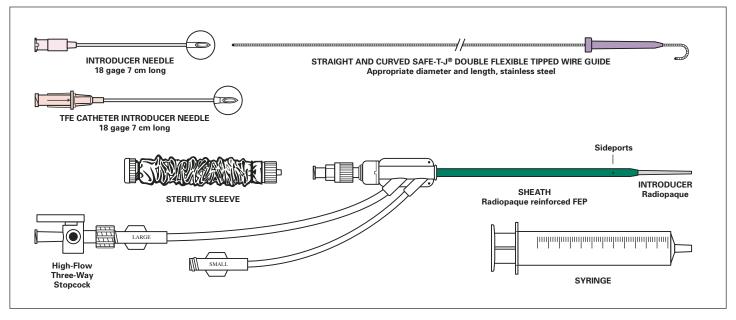

ORDER	<sup>1</sup> INTRODUCER	WIRE	GUIDE	SHEATH	Global Product
NUMBER	French Size	Diameter	Тір	Length	Number
Tray <sup>2</sup>					
C-DYBLIY-8.5-35-J-10.5	8.5	.035 inch	straight and 3 mm "J"	10.5 cm	G26909


<sup>&</sup>lt;sup>2</sup>Tray consists of items shown above and the following items: 25 gage needle, 22 gage needle, lidocaine, povidone-iodine swabsticks, fenestrated drape, gauze sponges, disposable syringe, disposable scalpel, suture with needle, povidone-iodine ointment, CSR wrap and prep tray.

#### **CHECK-FLO® PERFORMER® ACCESSORY ADAPTER**



- The accessory adapter can be connected to the proximal end of any Desilets-Hoffman sheath.
- The self-adjusting valve in the adapter prevents blood reflux and air aspiration during the introduction of catheters or instruments.
- The side-connection line can be used for flushing or as a second infusion line.

Supplied sterile in peel-open packages. Intended for one-time use.

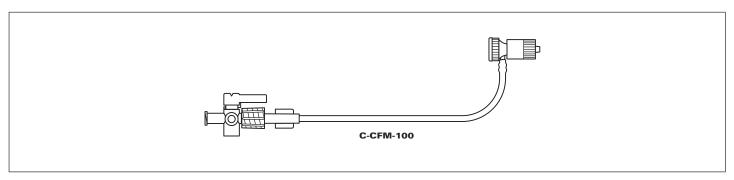


ORDER NUMBER	Accepts	Remarks	Global Product Number
C-CFM-100	3.0 thru 9.0 French	Check-Flo® Performer® valve to male Luer lock with side-connection line and three-way stopcock	G05149

Patent Pending

#### **STERILITY SLEEVE**




Used to help maintain the sterility of catheters or other instruments introduced through Check-Flo® Performer® and Tuohy-Borst sheaths. Accepts catheters or other instruments 3.0 to 9.0 French.Supplied sterile in peel-open packages. Intended for one-time use.

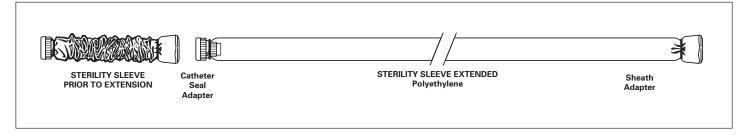

ORDER NUMBER	Length	Used With	Global Product Number
C-SPS-65-CK	65 cm	Check-Flo® Performer® sheath	G03611

U.S. Patent Numbers 4,551,137; 4,634,433

#### **PEEL-AWAY® INTRODUCER SETS**




Used for percutaneous introduction of balloon, electrode and closed or non-tapered end catheters for vascular and non-vascular use.

- Applications include placement of Permanent Pacemaker Leads, TPN Catheters, Silicone Central Venous Catheters, Hemodialysis Catheters, Tenckhoff Peritoneal Dialysis Catheters, Chest Drainage Tubes and Gastrostomy Catheters.
- The dual knobs allow the sheath to be peeled away and removed.

The maximum diameter of the instrument or catheter to be introduced should be determined to insure its passage through the sheath.1

Supplied sterile in peel-open packages. Intended for one-time use.

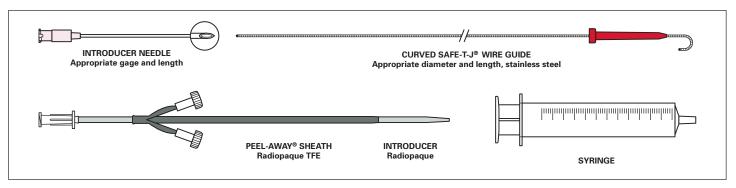

ORDER NUMBER	<sup>1</sup> INTRODUCER French Size	WIRE GUIDE Diameter	SHEATH Length	INTRODUCER Length	Global Product Number
Sets Pediatric					
C-PLIP-3.5-18	3.5	.018 inch	7 cm	11 cm	G03032
C-PLIP-4.0-21	4.0	.021 inch	7 cm	11 cm	G04116
C-PLIP-4.5-21	4.5	.021 inch	7 cm	11 cm	G02325
C-PLIP-5.0-25	5.0	.025 inch	9 cm	13 cm	G02916
C-PLIP-5.5-25	5.5	.025 inch	9 cm	13 cm	G05513
C-PLIP-6.0-35	6.0	.035 inch	9 cm	13 cm	G04117
C-PLIP-7.0-35	7.0	.035 inch	9 cm	13 cm	G04362
Standard					
C-PLI-7.0-35	7.0	.035 inch	15.5 cm	20 cm	G02187
C-PLI-8.0-38	8.0	.038 inch	15.5 cm	20 cm	G01922
C-PLI-9.0-38	9.0	.038 inch	15.5 cm	20 cm	G04502
C-PLI-10.0-38	10.0	.038 inch	15.5 cm	20 cm	G04495
C-PLI-11.0-38	11.0	.038 inch	15.5 cm	20 cm	G04496
C-PLI-12.0-38	12.0	.038 inch	15.5 cm	20 cm	G04497
C-PLI-13.0-38	13.0	.038 inch	15.5 cm	20 cm	G04498
C-PLI-14.0-38	14.0	.038 inch	15.5 cm	20 cm	G04499
C-PLI-16.0-38	16.0	.038 inch	15.5 cm	20 cm	G04500
C-PLI-18.0-38	18.0	.038 inch	15.5 cm	20 cm	G04501
C-PLI-20.0-38	20.0	.038 inch	13 cm	20 cm	G04509
C-PLI-22.0-38	22.0	.038 inch	13 cm	20 cm	G04518
C-PLI-24.0-38	24.0	.038 inch	13 cm	20 cm	G04511
C-PLI-26.0-38	26.0	.038 inch	13 cm	20 cm	G04840

#### **REFERENCES**

R. H. Dailey: "Use of Wire-Guided (Seldinger-Type) Catheters in the Emergency Department," *Annals of Emergency Medicine*, 12 (1983), 489-492.

B. E. Haynes, F. J. Carr, J. T. Niemann: "Catheter Introducers for Rapid Fluid Resuscitation," *Annals of Emergency Medicine*, 12 (1983), 606-609.

R. H. Dailey: "'Code Red' Protocol for Resuscitation of the Exsanguinated Patient," *Journal of Emergency Medicine*, 2 (1985), 373-378.

#### **VIDEOTAPES**

### C-VC-1 INTRODUCER TECHNIQUE FOR PLACEMENT OF PERMANENT PACEMAKER ELECTRODES

Author: J. Messenger, Memorial Hospital, Long Beach, California. (Duration: 13 minutes)

#### C-VC-7 PEEL-AWAY® SHEATH TECHNIQUE FOR PLACING PERITONEAL DIALYSIS CATHETERS

Author: S. Updike, University of Wisconsin Medical Center, Madison, Wisconsin. (Duration: 17 minutes)

#### C-VC-8 SILICONE RUBBER CATHETER (SILASTIC HYPERALIMENTATION)

Author: M. W. L. Gauderer, University Hospital, Cleveland, Ohio. (Duration: 15 minutes)



**Interventional Critical Care Products** 

www.cookcriticalcare.com

#### Distributed by:

COOK MEDICAL INCORPORATED

Phone: 812 339-2235, Toll Free: 800 457-4500, Toll Free Fax: 800 554-8335

COOK (CANADA) INC.

111 Sandiford Drive, Stouffville, Ontario, L4A 7X5 CANADA Phone: 905 640-7110, Toll Free: 800 668-0300

WILLIAM A. COOK AUSTRALIA PTY. LTD.

Brisbane Technology Park, 12 Electronics Street, Eight Mile Plains Brisbane, QLD 4113 AUSTRALIA, Phone: +61 7 38 41 11 88

WILLIAM COOK EUROPE ApS
Sandet 6, DK-4632, Bjaeverskov, DENMARK, Phone: +45 56 86 86 86

© COOK INCORPORATED 2005